

Fine particle measuring system

testo 380 – The innovative complete solution

In combination with testo 330-2 LL, the innovative complete solution for solid fuels, oil and gas systems.

Unrestricted TÜV test for the limit value levels 1/2 and according to VDI 4206 Sheet 2


Parallel measurement of fine particles, O₂ und CO

Graphic presentation of all measurement values in real time

Especially economic in operation and maintenance

Effortless handling and easy transport

High-tech in a case: Measurement of all relevant values with only one probe




The constantly growing number of solid fuel systems leads to a further increase in the emission of fine particles. The new amendment to the 1. BImSchV prescribes fine particle measurement, presenting chimneysweeps, heating constructors and service technicians with new challenges. With the new fine particle measuring system testo 380, fine particles can for the first time be measured simply on site. The completely new measurement method developed by Testo enables easy monitoring and implementation of the fine particle limit values. Combustion systems can be optimized to minimum emissions with the system.

The „command centre“ of the testo 380 is the proven emission analyzer testo 330-2 LL. When you take it out of the case, you can as usual determine, among other things, flue gas, flue draught and pressure on gas and oil systems. In connection with the testo 380, the simultaneous measurement of O₂, CO and fine particles is possible for the first time.

Overview of the measurement system

The fine particle measuring system testo 380 consists of two system components: the fine particle analyzer testo 380 including fine particle probe, and the testo 330-2 LL as a command centre and a flue gas analyzer. Together, this system offers the highest possible level of compactness, ease of handling and precision in the measurement of solid fuel, oil and gas systems.

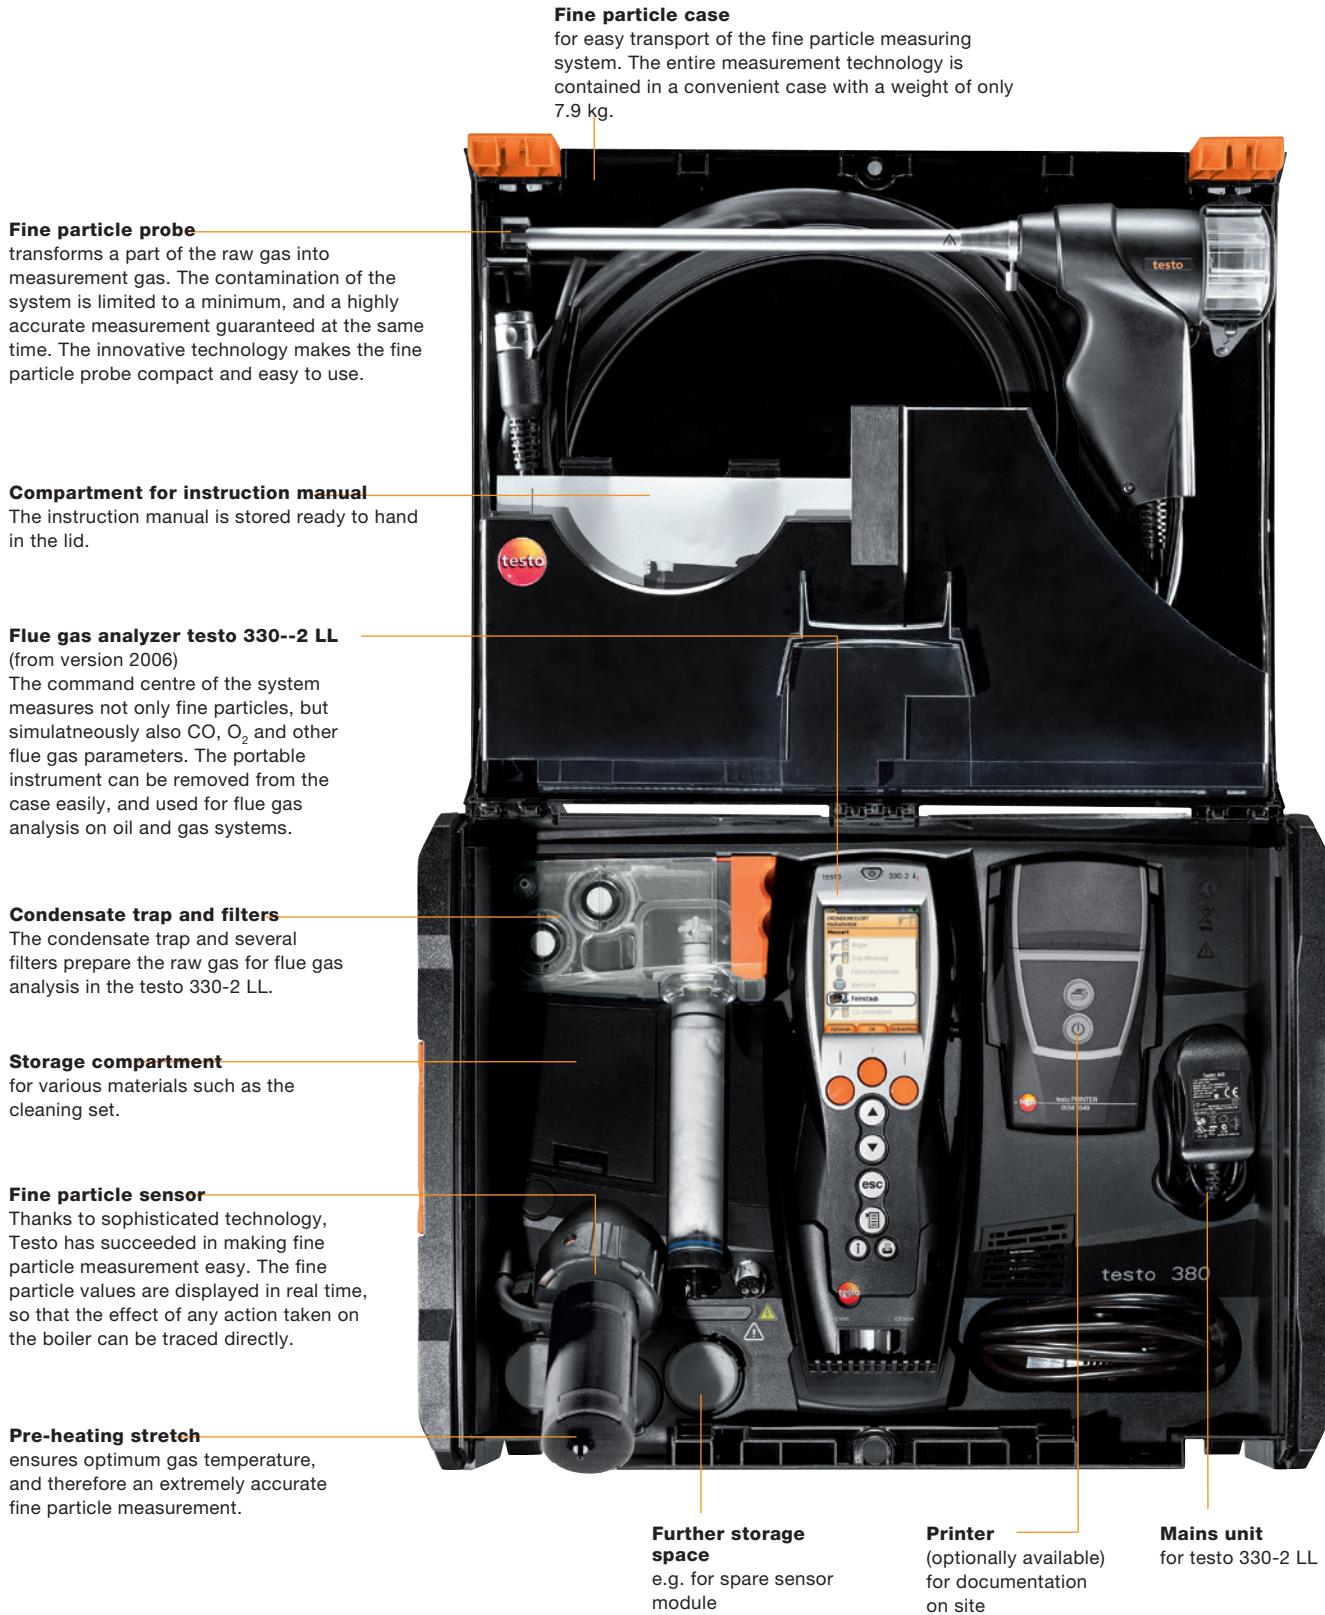



Innovative technology

The fine particle probe

Everything you need for your professional fine particle measurement is contained in Testo's own development, the handy fine particle probe. The probe samples the raw gas directly from the flue gas flow and transports it to the testo 330-2 LL for flue gas analysis. Simultaneously, the raw gas is mixed with fresh air in the rotation diluter – creating the necessary measurement gas for the fine particle measurement. The fine particle probe is also responsible for the measurement of the flue gas temperature and the flue draught. The probe is equipped with a heating element which ensures a constant temperature of 120 °C, in order that the flue gas does not condense during the measurement. The probe can be quickly and effortlessly stored in the measurement box, and just as easily removed again. Other probes are not necessary for the measurement of fine particles.



The rotation diluter

In order to achieve an especially reliable fine particle measurement, the raw gas is passed through a rotation diluter made of technical ceramics. Thanks to the patented technology, the particle concentration is diluted with the help of a defined quantity of fresh air, so that the contamination of the gas paths and the entire measurement system is reduced to a minimum, and at the same time a precise fine particle measurement takes place. This means the system works without deterioration, cleaning takes place using conventional household cotton buds.

The fine particle sensor

The fine particle sensor measures the mass of the particles contained in the measurement gas. For this purpose, the measurement gas is passed on to the oscillating fine particle sensor through a jet. Depending on the mass of the particles deposited, the oscillation frequency changes, thus allowing the particle mass to be determined. Because this calculation can be carried out at very short intervals thanks to Testo technology*, it is possible to follow the measurement values in the display of the testo 330-2 LL in real time during the entire duration of the measurement. This way, no smoke input is ever missed, any change in the heating boiler and its effects are immediately visible, and the system can be adjusted especially quickly and efficiently.

* several patents pending

Ordering data

testo 380 fine particle analyzer

- Without flue gas analyzer testo 330-2 LL (already owned testo 330-2 LL from version 2010 can be used after a Firmware update)

Part no. 0632 3800



testo 380 fine particle measuring system

- testo 380 fine particle analyzer with fine particle probe and cleaning set
- Flue gas analyzer testo 330-2 LL with mains unit (incl. Bluetooth, H₂-compensated CO cell)
- Modular flue gas probe 300 mm
- Combustion air temperature probe 190 mm

Part no. 0632 3801



Accessories

Flue gas analyzer testo 330-2 LL

Bluetooth testo 330-2 LL flue gas analyzer set with Longlife gas sensors; BLUETOOTH® and H₂-compensated CO sensor as well as integrated draught and gas zeroing, incl. rech. battery and calibration protocol; with graphic display

Part no.

0632 3307 70

Accessories testo 380

Part no.

testo 606-2 wood and material humidity meter with integrated humidity measurement and NTC air thermometer incl. protection cap, batteries, belt holder and calibration protocol, TÜV permit according to VDI 4206 page 4

0560 6062

Combustion air temperature probe, immersion depth 190 mm

0600 9787

testo 317-3 CO monitor, incl. carrying case with belt clip, headphones, wrist strap, sampler and calibration protocol

0632 3173

Testo fast printer IrDA with wireless infrared interface; 1 roll thermal paper; 4 AA batteries

0554 0549

Testo Bluetooth®/IRDA printer incl. 1 roll of printer paper, rechargeable battery and mains unit

0554 0620

Spare thermal paper for printer, permanent ink

0554 0568

easyheat PC analysis software, shows measurement in form of diagrams, tables and manages customer data.

0554 3332

USB connection cable instrument-PC, length 2 m

0449 0047

Spare parts testo 380

Part no.

Spare fine particle sensor module

0394 0001

Spare jet

0394 0002

Spare particle filter for testo 350 analyzer box (20 pcs.)

0554 3381

Probe attachment chain

0554 9356

Probe cleaning brush

0554 0228

Probes and accessories testo 330-2 LL

Retrofits / spare gas sensors

	Part no.
O ₂ sensor for testo 330-1 LL/-2 LL	0393 0002
CO sensor (without H ₂ -compensation) for testo 330-1 LL/-2 LL	0393 0061
CO sensor, H ₂ -compensated, 0 to 8000 ppm for testo 330-1 LL/-2 LL	0393 0101
Spare CO _{low} sensor for testo 330-1 LL/-2 LL	0393 0103
Spare NO sensor, 0 to 3000 ppm for testo 330-1 LL/-2 LL	0393 0151
Upgrade NO-sensor; 0 to 3000 ppm; resolution 1 ppm	0554 2151
NO _{low} spare sensor 0 to 300 ppm, 0.1 ppm, ±2 ppm (0 to 39.9 ppm) ±5% of m.v.	0393 0152



Modular flue gas probes

	Part no.
Flue gas probe modular, incl. cone for attachment; thermocouple NiCr-Ni; hose 2.2 m; particle filter; length 180 mm; Ø 8 mm; Tmax. 500 °C; TÜV-tested	0600 9760
Flue gas probe; length 300 mm; Ø 8 mm; Tmax. 500 °C; TÜV approval; probe stop; NiCr-Ni thermocouple; 2.2 m hose and particle filter included	0600 9761
Flue gas probe; length 180 mm; Ø 6 mm; Tmax. 500 °C; probe stop; NiCr-Ni thermocouple; 2.2 m hose and particle filter included	0600 9762
Flue gas probe; length 300 mm; Ø 6 mm; Tmax. 500 °C; probe stop; NiCr-Ni thermocouple; 2.2 m hose and particle filter included	0600 9763
Flue gas probe flexible; thermocouple NiCr-Ni; hose 2.2 m; dirt filter; length 330 mm; Ø 9 mm; Tmax. 180 °C; short-term 200 °C; ideal for measuring at inaccessible points	0600 9770

Probe accessories

	Part no.
Probe shaft; length 180 mm; 8 mm; Tmax. 500 °C	0554 9760
Probe shaft; length 300 mm; Ø 8 mm; Tmax. 500 °C	0554 9761
Probe shaft, length 335 mm, incl. cone, Ø 8 mm, Tmax 1000 °C	0554 8764
Probe shaft flexible; length 330 mm; Ø 9 mm; Tmax. 180 °C	0554 9770
Probe shaft multi-hole; length 300 mm; Ø 8 mm; for mean CO calculation	0554 5762
Probe shaft multi-hole; length 180 mm; Ø 8 mm; for mean CO calculation	0554 5763
Hose extension; 2.8 m; extension cable for probe	0554 1202
Probe stop 8 mm; steel; with spring clamp and handle; Tmax. 500 °C	0554 3330
Probe stop 6 mm; steel; with spring clamp and handle; Tmax. 500 °C	0554 3329

Additional probes

	Part no.
Dual wall clearance probe for O ₂ supply air measurement	0632 1260
Gas leak detection probe; 0 to 10000 ppm CH ₄ /C ₃ H ₈	0632 3330
Ambient CO probe, for detecting CO in buildings and rooms; 0 to +500 ppm	0632 3331
Connection cable for ambient CO ₂ probe	0430 0143
Fine pressure probe: highly accurate probe for the measurement of differential pressure and temperature, as well as Pitot tube measurement of flow velocities (see technical data)	0638 0330

Probes and accessories testo 330-2 LL

Combustion air temperature probes

Part no.

Combustion air temperature probe, immersion depth 190 mm	0600 9787	
Combustion air temperature probe, immersion depth 60 mm	0600 9797	

Additional temperature probes

Part no.

Mini ambient air probe; for separate ambient air temperature measurement; 0 to +80 °C	0600 3692	
Very fast reaction surface probe	0604 0194	
Connection cable	0430 0143	

Accessories testo 330-2 LL

Part no.

Mains unit international 100-240 V AC / 6.3 V DC for mains operation or battery charging in instrument	0554 1096	
Spare battery 2600 mA	0515 5107	
Smoke tester with oil and soot sheet, for measuring soot in flue gas, excl. cone (part no. 0554 9010)	0554 0307	
Hose connection set with adapter for separate gas pressure measurement	0554 1203	
Pressure set for testing gas line testo 330-1/-2 LL version 2010	0554 1213	
Differential temperature set; consisting of 2 Velcro probes and temperature adapter	0554 1208	
Spare dirt filter, modular probe; 10 off	0554 3385	
easyheat PC analysis software, shows measurement in form of diagrams, tables and manages customer data.	0554 3332	
USB connection cable instrument to PC testo 330-1/-2 LL / testo 335	0449 0047	
ISO calibration certificate/flue gas	0520 0055	

Technical data

Measuring range, accuracy, resolution

Measuring range	0 to 300 mg/m ³
Accuracy	acc. VDI 4206-2
Resolution	0.1 mg/m ³ (>5mg/m ³)
Memory	500.000 readings

Other instrument information

Storage and transport temperature	-20 to +50 °C
Operating temperature	+5 to +40 °C
Protection class	IP40
Weight	testo 380: 7.9 kg, testo 330-2 LL: 0.65 kg
Dimensions	475 x 360 x 190 mm
Housing material	ABS
Power supply	via internal mains unit: 100 V AC/0.45 A to 240 V AC/0.2 A (50 to 60 Hz)
Power consumption	max. 100 W

Information fine particle probe

Probe length	270 mm
Probe shaft diameter	12 mm
Probe shaft material	Stainless steel 1.4301
Probe cable length	2.2 m
Integrated elements	Draught measurement, sampling, temperature measurement, probe heating, rotation diluter
Flue gas temperature	max. +500 °C
Probe shaft heating	to +120 °C
Rotation diluter	heated up to +80 °C
Status display	LED, shows warm-up phase and operational readiness